


User Instruction Manual

Oxford® Quickfit Sling

To avoid injury, read user manual prior to use. For alternative languages, contact your authorised service provider.

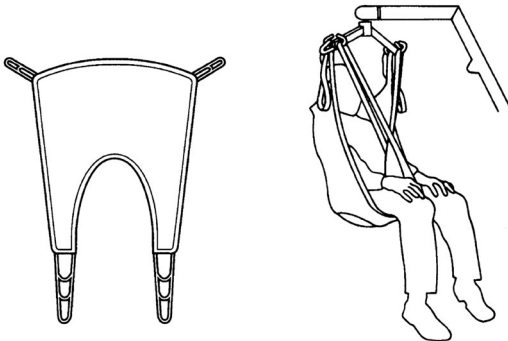

Introduction

The Oxford® Quickfit sling is an easy to fit general-purpose, sling with divided leg sections, designed to suit around 85% of clients. The Quickfit design has become one of the most recognised sling choices available today. Available in a choice of material options.

Special Sling Orders

On occasions, material, dimensional and other changes outside of the standard specification are requested. Please be advised, that aside of any model specific references, fitting, washing and safety guidelines remain applicable. If you are in any doubt, please contact your authorised Oxford service agent or Joerns Healthcare directly.

Statement of Intended Use

A sling is an item of moving and handling equipment that is used with a mechanical lift in order to facilitate the transfer of a patient. It comprises a specially designed and constructed piece of fabric that is placed under and/or around a patient before being attached to the spreader bar/cradle of a lift to raise, transfer and lower the patient. When selected and used correctly, a sling and lift combination will achieve a safer transfer and reduce the risks associated with manual handling.

It is the responsibility of a competent person to conduct a thorough risk assessment prior to using any sling, to ensure that the sling choice, method of positioning in the sling and procedure for transfer has been correctly determined for the patient. For further guidance, please contact your authorised Oxford Service Provider or Joerns Healthcare.

FOR USE WITH PASSIVE LIFTS ONLY.

Expected Service Life

The expected service life of an Oxford sling will vary dependent on use and following the care and washing instructions provided in the user guide. Factors such as wash temperature, detergents, frequency of use and patient weight will impact on the lifetime of your sling. Joerns Healthcare recommend that slings are checked each and every time prior to use to ensure the safety of the patient. Bleached, torn, cut, frayed or broken slings are unsafe and must be discarded and replaced. It is a requirement under LOLER (Lifting Operations and Lifting Equipment Regulations 1998) that slings are thoroughly checked and passed fit for use. For further advice, please contact your authorised Oxford Service Provider or Joerns Healthcare.


Serious Incident Reporting

In the event of a serious incident taking place during use of this product, affecting the patient and/or caregiver, it must be reported to the product manufacturer or authorised distributor. Should the incident take place within the European Union (EU), it must also be reported to the local competent authority within the member state.


▲ WARNING

- **OXFORD RECOMMENDS THE USE OF GENUINE OXFORD PARTS.** Oxford sling and lift products are designed to be compatible with one another. For country specific guidance on sling use and compatibility, please refer to the sling label or contact your local market distributor or Joerns Healthcare.
- For the safety of the patient and carer; before using a sling a full risk assessment must be conducted to ensure that the correct sling choice, method of positioning in the sling and procedure for transfer has been determined for the patient.
- **CHECK** sling and stitching before each use. Using bleached, torn, cut, frayed or broken slings is unsafe and could result in serious injury or death to the patient.
- **DO NOT** alter slings. Destroy and discard worn slings.
- **NEVER** leave a patient unattended.
- **DO NOT** exceed the rated capacity of the sling or lift.
- **DO NOT** attempt to re-position a patient by pulling on the sling loops.


Fitting the Sling from a Seated Position

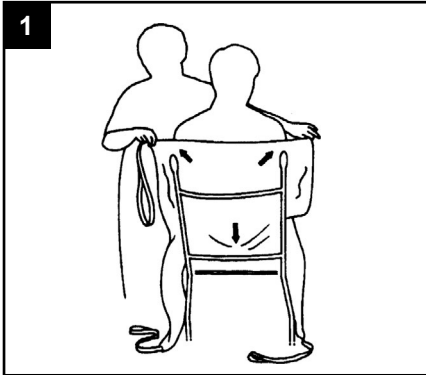


Ensure the sling positioning handles and label are on the outside and feed the sling down the back of the client, leaving the lower edge of the sling body at the base of the spine. Check the sling is square at the shoulders.

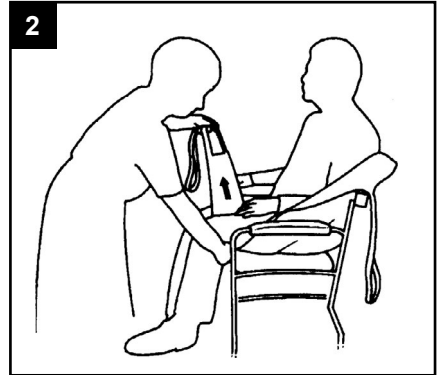

Raise the client's leg and carefully feed the leg section under and up between the legs. Ensure that the sling is positioned comfortably and not twisted or creased under the thigh. Repeat this procedure for the other leg.

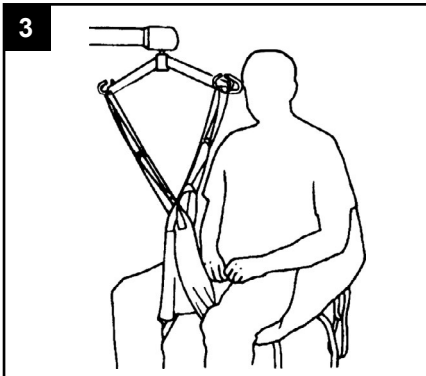


Move the hoist into position before crossing over the leg straps and attaching to the hoist on the front hooks of the spreader bar. An integrated modesty loop on the leg section is also available for increased patient dignity.

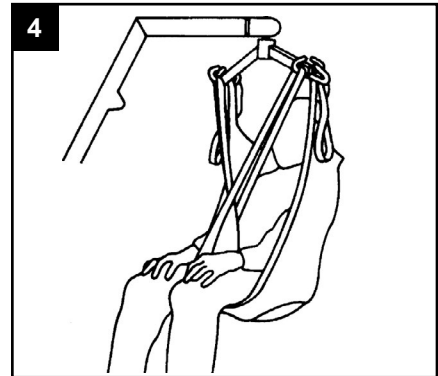

Ensure the sling remains comfortable under the legs and raise the hoist slightly if required before attaching the shoulder straps to maintain an upright seated position. The hoist may move towards the client as you do this. When re-seating the client, use the sling positioning handles to help achieve a safe and comfortable position.

NOTE: Sling positioning handles are designed for turning a patient only and must not be used for lifting.

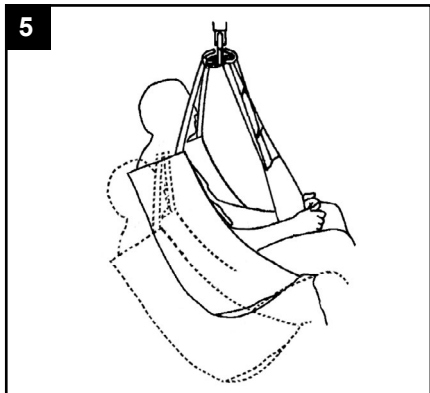


The longer you attach the shoulder straps, the more reclined the client will be.

GOLDEN RULE:

In order to achieve an upright seated position, go long with the leg straps and short with the shoulder straps.


Fitting the Sling from a Lying Position

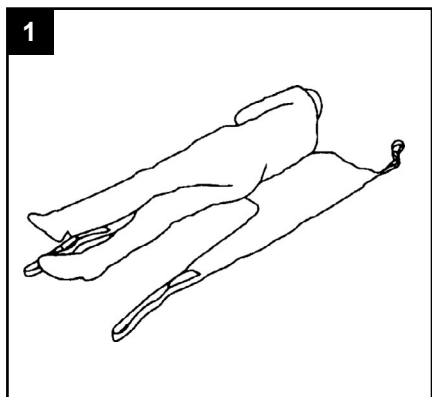

Safely position the client onto the sling, ensuring that the lower edge of the sling body is positioned at the base of the spine.

NOTE: For added safety and support, Joerns Healthcare recommend the use of a head support when lifting from the floor.

IMPORTANT: ENSURE THAT YOUR CLIENT'S HEAD IS SUPPORTED AT ALL TIMES

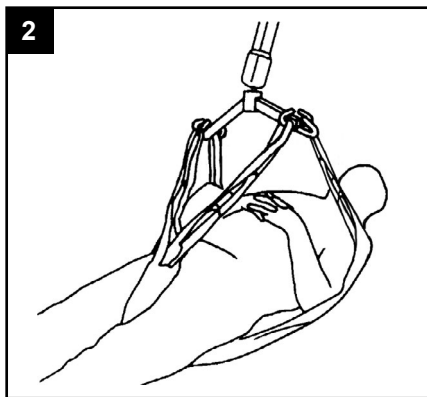

Carefully feed the leg sections under and up between the legs, ensuring that the sling is positioned comfortably and not twisted or creased under the thigh. Cross the leg straps, using the modesty loop if required and proceed to attach the sling to the spreader bar in the same manner as with the seated position.

NOTE: The longer you attach the shoulder straps, the more reclined the client will be.

Technical Specifications

| | |
|----------|-----------------|
| STANDARD | BS EN ISO 10535 |
|----------|-----------------|

Sizing & Safe Working Load

| SIZE | Quickfit (Polyester) | Quickfit (Net) | Quickfit (Spacer) | Quickfit Padded (Polyester) |
|--------------------|----------------------|----------------|-------------------|-----------------------------|
| PAEDIATRIC (BROWN) | 500lbs / 227kg | 500lbs / 227kg | 500lbs / 227kg | 500lbs / 227kg |
| SMALL (RED) | 500lbs / 227kg | 500lbs / 227kg | 500lbs / 227kg | 500lbs / 227kg |
| MEDIUM (YELLOW) | 500lbs / 227kg | 500lbs / 227kg | 500lbs / 227kg | 500lbs / 227kg |
| LARGE (GREEN) | 500lbs / 227kg | 500lbs / 227kg | 500lbs / 227kg | 500lbs / 227kg |
| EXTRA LARGE (BLUE) | 500lbs / 227kg | 500lbs / 227kg | 500lbs / 227kg | 500lbs / 227kg |

For more information on sling dimensions, please contact us. For guidance on sling application, visit www.oxfordslingsselector.co.uk.

Key Symbols

The following symbols are used for the Oxford Full Back Sling.



This product is a Medical Device in accordance with EU Medical Device Regulation 2017/745.



ATTENTION, consult accompanying documents.



Refer to the user instructions before use.



Certification mark indicating conformity with the applicable requirements for products sold within Great Britain.



A point of contact between the non-European medical device manufacturer, the national Competent Authorities (Ministry of Health) and Notified Bodies.



A unique device identification intended to provide single, globally harmonised positive identification of medical devices through distribution and use.



Indicates the entity importing the medical device into the locale.

Washing Instructions & Safety Checks



Machine wash at 85°C.



DO NOT wash with bleach. Bleach will damage the sling's material and make it unsafe for use.



Cool tumble dry, air dry or dry at very low temperature.



DO NOT dry clean.



⚠ WARNING

Slings can suffer damage during washing and drying and should be checked carefully before each use. Scan QR code or [click here](#) for important sling safety checks and information.

PLEASE NOTE: Additional slings are available to meet individual patient needs. We advise that you always seek the advice of a trained clinician, authorised Oxford distributor or Joerns Healthcare prior to purchase or use.

End of Life Disposal

Slings and associated material accessories should be sorted as combustible waste in accordance with local or national regulations.

Istruzioni di lavaggio & Controlli di sicurezza



Lavatrice a 85°C.



NON lavare con candeggina. La candeggina potrebbe danneggiare il materiale delle imbracature e renderle pericolose all'utilizzo.



Asciugare in asciugatrice, all'aria aperta o temperature molto basse.



NON lavare a secco.



⚠ AVVERTENZE

Le imbracature potrebbero danneggiarsi durante il lavaggio e l'asciugatura e dovrebbero essere controllate con cura prima di ogni utilizzo. Scannerizza il QR code o [clicca qui](#) per importanti controlli di sicurezza e informazioni.

NOTA BENE: Imbracature addizionali sono disponibili ad incontrare le singole esigenze dei pazienti. Consigliamo di chiedere sempre il parere di un medico qualificato, un distributore Oxford autorizzato oppure direttamente Joerns Healthcare per l'acquisto o l'utilizzo.

Fine vita del dispositivo

Le imbracature e gli accessori ad esse associati dovrebbero essere smatite come rifiuti combustibili in conformità con le normative locali o nazionali



Special Products and Service

Contact Us

Units 5 and 6 Lower Vicarage
Road

Southampton
Hampshire

SO19 7RJ

T: 02380 420678

E: info@easycareystems.co.uk

www.easycareystems.co.uk